

**Project Acronym:**  
FUSVET (SEED/1221/0080)

Focused Ultrasound System for veterinary chemotherapeutic applications for oncology

**Deliverable number: 2.1**

**Title:** Presentation at a scientific conference

**Prepared by:**

Anastasia Antoniou (CUT)  
Christakis Damianou (CUT)

**Date:** 31/10/2023



**Ευρωπαϊκή Ένωση**  
Ευρωπαϊκά Διαρθρωτικά  
και Επενδυτικά Ταμεία



Κυπριακή Δημοκρατία



**Διαρθρωτικά Ταμεία**  
της Ευρωπαϊκής Ένωσης στην Κύπρο

## Table of Contents

<b>Executive summary</b> .....	3
<b>Submitted abstracts</b> .....	5
<b>Appendix: Oral and Poster presentations given</b> .....	13

## **Executive summary**

This deliverable presents the Conference papers that were presented during the 1<sup>st</sup> reporting period of the FUSVET project. The papers covered multiple topics in the area of Magnetic Resonance Imaging (MRI)-guided FUS (MRgFUS), including but not limited to the development of tumor-bearing tissue mimicking phantoms and robotic systems for veterinary applications, and the treatment of naturally occurring mammary tumors in pets by FUS ablation. Caution was given to avoid disclosing any key features and components of the FUSVET system prior to the relevant patent application.

Table 1 provides details on each paper, including its title and presentation format (oral or poster), and the relevant conference where it was presented. The oral and poster presentations can be found in the Appendix in the same order as in Table 1.

It is noted that some of the research work carried out under the FUSVET project was a synergy with the SOUNDPET project (running at the same time).

**Table 1:** List of conference papers presented during the 1s reporting period of the **FUSVET** project.

#	Title	Conference	Date	Type	Online/ In-person
1	Focused Ultrasound Ablation Of Canine Mammary Cancer	<i>UltraCon Annual Meeting 2023, Orlando, Florida, USA</i>	25-29 March 2023	Poster	In person
2	Focused Ultrasound Phantom With Inclusion Of Tumour	<i>UltraCon Annual Meeting 2023, Orlando, Florida</i>	25-29 March 2023	Poster	In person
3	MRI guided focused ultrasound system for veterinary oncology	<i>12th Veterinary Forum on companion animal medicine, Thessaloniki, Greece</i>	01-02 April 2023	Poster	In person
4	T1 and T2 values of an Agar-based phantom with inclusion of tumour	<i>12th Veterinary Forum on companion animal medicine, Thessaloniki, Greece</i>	01-02 April 2023	Poster	In person
5	Treatment of cancer with focused Ultrasound in cats and dogs	<i>The 22nd Annual International Symposium on Therapeutic Ultrasound (ISTU), Lyon, France</i>	17-20 April 2023	Poster	In person
6	Ultrasound and MRI guided focused ultrasound system for veterinary applications	<i>The 29th annual international conference of the Australian sonographers association, Brisbane, Australia</i>	26-28 May 2023	Oral	In person
7	MR thermometry for a multipurpose phantom for focused ultrasound	<i>6th International Caparica Conference on Ultrasonic-based applications from analysis to synthesis, Caparica, Portugal</i>	26–29 June 2023	Poster	In person
8	Robotic system for veterinary applications	<i>6th International Conference on Manipulation, Automation and Robotics at Small Scales (MARSS), Abu Dhabi, UAE</i>	09-13 October 2023	Oral	In person

## **Submitted abstracts**

### ***1. UltraCon Annual Meeting 2023, Orlando, Florida, USA***

#### **Focused Ultrasound Ablation Of Canine Mammary Cancer**

Anastasia Antoniou, Nikolas Evripidou, Christakis Damianou\*

Department of Electrical Engineering, Computer Engineering, and Informatics, Cyprus University of Technology, Limassol, Cyprus.

\* *Corresponding author. email: [christakis.damianou@cut.ac.cy](mailto:christakis.damianou@cut.ac.cy)*

#### **ABSTRACT**

##### ***Objectives***

Veterinary medicine is continuously expanding its applications beyond traditional approaches. In this regard, the Focused Ultrasound (FUS) technology has many potential applications, including tumor destruction, drug delivery, pain relief, and noninvasive spaying. The current study examined the feasibility of FUS in the treatment of naturally occurring canine superficial mammary cancer using an existing preclinical MRI-compatible FUS robotic system.

##### ***Methods***

The robotic system utilized comprises a positioning mechanism for navigating a single element spherically focused transducer of 2.6 MHz in four PC-controlled axes. For each cage dog (n=5), the system was installed in the respective veterinary clinic. The dog was comfortably positioned on the device so that the tumour is located in the acoustic opening directly above the FUS transducer. Degassed water was used for ultrasonic coupling. The treatment protocol was adjusted based on the tumour size and location. The motion and ultrasonic parameters were controlled through dedicated FUS software. Post-sonication the tumours were removed and sent for histological examination.

##### ***Results***

All procedures were implemented successfully, with no recorded adverse events compromising pet welfare. Hematoxylin and eosin (H&E) staining demonstrated well-defined regions of coagulative necrosis in the treated tumours with no off-target damage, except from minor red blood cell extravasation observed in some cases at the borderline of thermal lesions.

##### ***Conclusions***

In this study, FUS ablation of canine mammary cancer under proper monitoring was proven safe and feasible. The FUS robotic system and related software offered an efficient procedural workflow. Veterinary clinical trials offer the opportunity for FUS to benefit family pets by providing them an alternative non-invasive cancer treatment.

## **2. UltraCon Annual Meeting 2023, Orlando, Florida, USA**

### **Focused Ultrasound Phantom With Inclusion Of Tumour**

Christakis Damianou\*, Anastasia Antoniou, Nikolas Evripidou

Department of Electrical Engineering, Computer Engineering, and Informatics, Cyprus University of Technology, Limassol, Cyprus.

\* *Corresponding author. email: [christakis.damianou@cut.ac.cy](mailto:christakis.damianou@cut.ac.cy)*

### **ABSTRACT**

#### ***Objectives***

An agar-based mimicking material which includes a tumour was developed. The phantom can be used to evaluate the temperature produced by a focused ultrasound transducer.

#### ***Methods***

The tumour model was made out of water, agar (6 % w/v) and 4 % w/v silica. In the tissue surrounding the tumour no silica was used.

#### ***Results***

The slight difference in silica content between tumour and surrounding tissue resulted in excellent contrast between tumour and tissue in Magnetic Resonance Imaging (MRI). Based on coronal images showing the transducer and tumour/tissue it was possible to precisely move the focused ultrasound beam within the phantom using an MR compatible positioning device. MR temperature was detected within the tumour and outside the tumour. T1 and T2 values were measured in a 3 T MRI.

#### ***Conclusions***

Due to the inclusion of silica in the tumour the absorption was increased within the tumour, and therefore, higher temperatures were measured in the tumour. Temperature across a plane parallel to the beam showed some deflection of the beam in areas of tumour curvature. This is an excellent tumour model that can be used to evaluate the physics of focused ultrasound.

### **3. 12th Veterinary Forum on companion animal medicine, Thessaloniki, Greece**

#### **MRI guided focused ultrasound system for veterinary oncology**

Damianou C.,<sup>1</sup> Spanoudes K.,<sup>2</sup>

<sup>1</sup>PhD, Professor, University of Technology, Limassol, Cyprus

<sup>2</sup>DVM, PhD student, VET EX MACHINA LTD, Nicosia, Cyprus

**Introduction:** In this paper Focused Ultrasound (FUS) technology was used for veterinary oncology applications. This modality is an additional tool beyond traditional approaches. In this study we investigated the ability of FUS to precisely ablate hypothetical targets mimicking canine and feline tumours

**Materials and methods:** Agar based targets were ablated with a Magnetic Resonance guided FUS (MRgFUS) robotic system featuring a single element spherically focused transducer of 2.7 MHz. The robotic system includes 3 linear cartesian axes.

**Results:** The MRgFUS system was capable of producing well-defined overlapping lesions in the mimicking tumours. The tumour mimicking phantom was imaged using MRI.

**Conclusions:** This technology has potential as a therapeutic solution for veterinary cancer. Although the device is MRI compatible, it can be used also outside the MRI setting using ultrasonic imaging. The next step is to apply this technology in animals and in humans.

**Reference:** Spanoudes K., Evripidou N., Giannakou M., Drakos T, Menikou G., Damianou C. (2021) A high intensity focused ultrasound system for veterinary oncology applications. J. Med. Ultrasound 29, 195-202.

#### ***4. 12th Veterinary Forum on companion animal medicine, Thessaloniki, Greece***

### **T1 and T2 values of an Agar-based phantom with inclusion of tumour**

Damianou C.,<sup>1</sup> Spanoudes K.,<sup>2</sup>

<sup>1</sup>PhD, Professor, University of Technology, Limassol, Cyprus

<sup>2</sup>DVM, PhD student, VET EX MACHINA LTD, Nicosia, Cyprus

**Introduction:** An agar-based mimicking material which includes a tumour was developed. The phantom can be used to evaluate the temperature produced by a focused ultrasound transducer.

**Materials and methods:** The tumour model was made out of water, agar (6 % w/v) and 4 % w/v silica. In the tissue surrounding the tumour no silica was used.

**Results:** The slight difference in silica content between tumour and surrounding tissue resulted in excellent contrast between tumour and tissue in Magnetic Resonance Imaging (MRI). Based on coronal images showing the transducer and tumour/tissue it was possible to precisely move the focused ultrasound beam within the phantom using an MR compatible positioning device. MR temperature was detected within the tumour and outside the tumour. T1 and T2 values were measured in a 3 T MRI.

**Conclusions:** Due to the inclusion of silica in the tumour the absorption was increased within the tumour, and therefore, higher temperatures were measured in the tumour. Temperature across a plane parallel to the beam showed some deflection of the beam in areas of tumour curvature. This is an excellent tumour model that can be used to evaluate the physics of focused ultrasound.

**Reference:** Antoniou, A., Damianou, C. (2022) Simple, inexpensive, and ergonomic phantom for quality assurance control of MRI guided Focused Ultrasound systems. J Ultrasound (<https://doi.org/10.1007/s40477-022-00740-w>)



**5. *The 22nd Annual International Symposium on Therapeutic Ultrasound (ISTU), Lyon, France***

**Treatment of cancer with focused Ultrasound in cats and dogs**

Anastasia Antoniou, Nikolas Evripidou, Kyriakos Spanoudes, Christakis Damianou

Department of Electrical Engineering, Computer Engineering, and Informatics,

Cyprus University of Technology, Limassol, Cyprus.

**ABSTRACT**

The current study is a feasibility study using MRI guided focused ultrasound (FUS) for the treatment of canine and feline cancer therapy.

FUS was delivered by a 2-MHz single-element spherically MRI compatible focused ultrasonic transducer which was integrated with an existing robotic positioning device. The functionality of the FUS system and sonication protocol in efficiently and safely ablating live tissue was initially validated in a rabbit thigh model in laboratory environment. The positioning device had 4 computer-controlled axes.

Eleven (11) referrals for dogs and cats with superficial mammary cancer were collected through a national recruitment champagne, from which 9 were considered to fulfill the set safety criteria. The eligible veterinary patients underwent FUS ablation followed by immediate surgical resection of the entire malignancy.

Histopathology examination demonstrated well-defined regions of coagulative necrosis in all treated tumors with no damage in the surrounding tissue. Further study with a larger patient population for other type of tumours is needed to confirm the findings and demonstrate the feasibility of thermal FUS to safely ablate deep seated tumors.

Keywords: high intensity focused ultrasound; mammary cancer; robotic device; thermal ablation; dogs; cats

**6. *The 29th annual international conference of the Australian sonographers association, Brisbane, Australia***

**Ultrasound and MRI guided focused ultrasound system for veterinary applications**

Nikolas Evripidou, Anastasia Antoniou, Christakis Damianou

Department of Electrical engineering, Computer engineering and Informatics, Cyprus  
University of Technology

*Objective: In this paper Focused Ultrasound (FUS) technology was used for oncology applications for veterinary applications. This modality is an additional tool beyond traditional approaches. In this study we investigated the ability of FUS to precisely ablate hypothetical targets mimicking canine and feline tumours*

*Material and methods:*

*Agar based targets were ablated with a Magnetic Resonance guided FUS (MRgFUS) robotic system featuring a single element spherically focused transducer of 2.7 MHz. The robotic system includes 3 linear cartesian axes.*

*Results*

*The MRgFUS system was capable of producing well-defined large lesions produced by navigating the transducer in a grid formation with 3 mm step in the mimicking tumours. The tumour mimicking phantom was imaged using ultrasound imaging and MRI.*

*Conclusions*

*This technology has potential as a therapeutic solution for veterinary cancer. Although the device is MRI compatible, it can be used also outside the MRI setting using ultrasonic imaging. The next step is to apply this technology in animals and in humans.*

**7. 6th International Caparica Conference on Ultrasonic-based applications from analysis to synthesis, Caparica, Portugal**

**MR thermometry for a multipurpose phantom for focused ultrasound**

**Christakis Damianou\*, Nikolas Evripidou, Andreas Georgiou**

Electrical Engineering Department, Cyprus University of Technology, Cyprus

\* christakis.damianou@cut.ac.cy

**Abstract**

Agar based phantoms were proven a valuable tool for preclinical MRI-guided Focused Ultrasound (MRgFUS) applications [1]. In this article we present our experience in acquiring thermal maps in a multipurpose phantom for a FUS system operated under MRI monitoring. An Agar based phantom was used as the background tissue. The phantom contained a cyst mimic, a bone mimic, a stone mimic and a tumour mimic. A single element transducer was used operating at 2.7 MHz. The robotic system included 3 cartesian axes (X,Y,Z) and one angular axis. A Siemens Magnetom 3 T MRI scanner was used. Temperature maps were acquired in the agar-based phantoms. The FLASH pulse sequence was optimized to provide noise-free temperature maps. It was found that the bone and stone mimic blocked ultrasound. The cyst mimic allowed ultrasound to pass through and the tumour mimic absorbed sufficient ultrasound. This inexpensive phantom was proven successful in studying the penetration of focused ultrasound through these mimics.

**References**

[1] McGarry, C.K. *et al.* Tissue mimicking materials for imaging and therapy phantoms: A review. *Physics in Medicine and Biology*, **2020**, 65. <https://doi.org/10.1088/1361-6560/abbd17>.

**Acknowledgements**

The study was co-funded by the European Structural & Investment Funds (ESIF) and the Republic of Cyprus through the Research and Innovation Foundation (RIF) under the projects SOUNDPET (INTEGRATED/0918/0008) and FUSVET (SEED/1221/0080).

**8. 6th International Conference on Manipulation, Automation and Robotics at Small Scales (MARSS), Abu Dhabi, UAE**

**Robotic system for veterinary applications**

Kyriakos Spanoudes<sup>a</sup>, Christakis Damianou<sup>b\*</sup>

<sup>a</sup> VET EX MACHINA, Larnaca, Cyprus

<sup>b</sup> Department of Electrical Engineering, Computer Engineering, and Informatics, Cyprus University of Technology, 30 Archbishop Kyprianou Street, 3036 Limassol, Cyprus.

**ABSTRACT**

This paper explores the use of Focused Ultrasound (FUS) technology for the treatment of cancer in pets (cats and dogs) using a specially designed robotic system with 3 cartesian axes and one angular axis. The system was designed to be Magnetic Resonance imaging (MRI) compatible. The positioning device includes a single element spherically focused transducer. The system was tested in agar-based phantoms and freshly excised tissue. This technology has potential as a therapeutic solution for veterinary cancer.

**KEYWORDS:** MRI, ultrasound, positioning device, dogs, cats

## **Appendix**

### **Oral and Poster presentations given**

# Focused Ultrasound Ablation Of Canine Mammary Cancer

A. Antoniou,<sup>1</sup> N. Evripidou,<sup>2</sup> C. Damianou<sup>\*3</sup>

*Electrical Engineering Department, Cyprus University of Technology, Cyprus*

<sup>1</sup> [anastasiaantoniou12@gmail.com](mailto:anastasiaantoniou12@gmail.com)

<sup>2</sup> [nk.evripidou@edu.cut.ac.cy](mailto:nk.evripidou@edu.cut.ac.cy)

<sup>3</sup> [christakis.damianou@cut.ac.cy](mailto:christakis.damianou@cut.ac.cy)

\* Corresponding author

ultracon

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

 Cyprus  
University of  
Technology

## INTRODUCTION

The current study examined the feasibility of Focused Ultrasound (FUS) in the treatment of naturally occurring canine superficial mammary cancer using an existing preclinical MRI-compatible FUS robotic system.



ultracon

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

## METHODS




The robotic system utilized comprises a positioning mechanism for navigating a single element spherically focused transducer of 2.6 MHz in four PC-controlled axes. For each case dog (n=5), the system was installed in the respective veterinary clinic.

The treatment protocol included partial tumor ablation and was adjusted based on the tumor size and location. The motion and ultrasonic parameters were controlled through dedicated FUS software. Post-sonication the tumors were removed and sent for histological examination.

## RESULTS

All procedures were implemented successfully, with no recorded adverse events. Hematoxylin and eosin (H&E) staining showed well-defined necrotic regions in all treated tumors. Red blood cell extravasation was observed at the lesion borderline in one case (1/5).

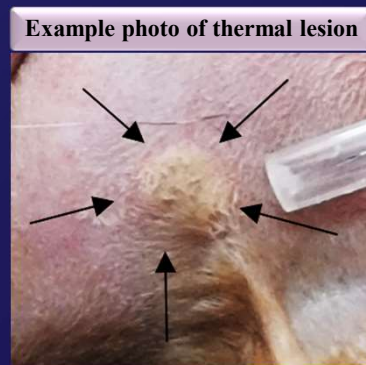


*Black arrows indicate thermal lesion inflicted on mammary tumor using 45-W acoustic power; focal intensity of 1590 W/cm<sup>2</sup> and sonication duration of 20 s.*


# RESULTS

## Indicative histological slides

Black arrows delineate the area of thermal necrosis.

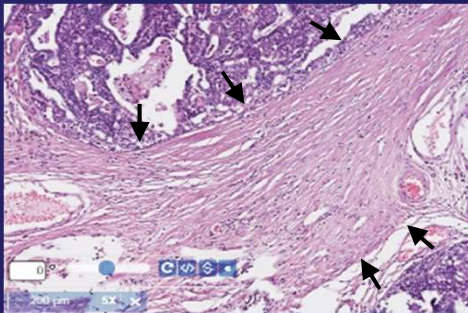


5X Magnification. Necrotic area created by sonication at 60 W; focal intensity of 2116 W/cm<sup>2</sup> for 10 s at 2.5-cm focal depth.

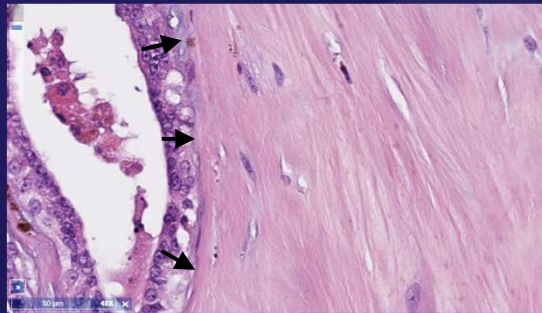


40X Magnification. Necrotic area created by sonication at 60 W; focal intensity of 2116 W/cm<sup>2</sup> for 10 s at 2.5-cm focal depth.

# RESULTS

## Indicative histological slides

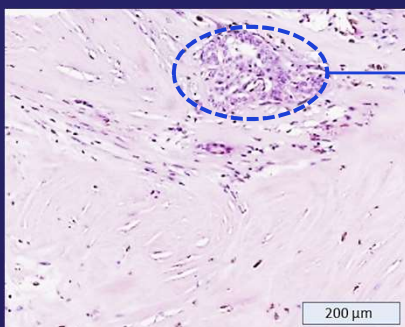

Intact cancer structure within the necrotic area.

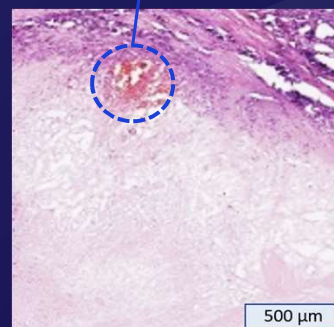

Minor hemorrhage observed at lesion borderline.



## CONCLUSIONS



FUS ablation of canine mammary cancer under proper monitoring was proven safe and feasible. The FUS robotic system and related software offered an efficient procedural workflow.

Further research is required to examine the phenomenon of residual cancer structures and the feasibility of safely ablating the entire tumor volume, as well as deep-seated tumors. Veterinary clinical trials may offer the opportunity for FUS to benefit family pets by providing them an alternative non-invasive cancer treatment.

ultracon

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

## ACKNOWLEDGEMENTS

The study was funded by the Research and Innovation Foundation  
of Cyprus under the projects:  
SOUNDPET (INTEGRATED/0918/0008)  
FUSVET (SEED/1221/0080)



ultracon

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

Cyprus  
University of  
Technology

# Focused Ultrasound Phantom With Inclusion Of Tumour

C. Damianou,<sup>\*1</sup> A. Antoniou,<sup>2</sup> N. Evripidou<sup>3</sup>

*Electrical Engineering Department, Cyprus University of Technology, Cyprus*

<sup>1</sup> [christakis.damianou@cut.ac.cy](mailto:christakis.damianou@cut.ac.cy)

<sup>2</sup> [anastasiaantoniou12@gmail.com](mailto:anastasiaantoniou12@gmail.com)

<sup>3</sup> [nk.evripidou@edu.cut.ac.cy](mailto:nk.evripidou@edu.cut.ac.cy)

\* Corresponding author

ultracon | AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

 Cyprus  
University of  
Technology

## INTRODUCTION

An agar-based tissue mimicking material which includes a tumour was developed. The phantom can be used to evaluate the temperature produced by a focused ultrasound (FUS) transducer.



ultracon | AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

## METHODS

The tumour model was made of water, agar (6 % w/v) and (4 % w/v) silica. In the material surrounding the tumour no silica was used.

The phantom was assessed in a 3T Magnetic Resonance Imaging (MRI) scanner in terms of T1 and T2 relaxation properties and overall MRI appearance. FUS sonications were performed in the phantom using an MR compatible positioning device to examine its response to thermal heating using MR thermometry.




Experimental setup for phantom sonication.

## RESULTS

The slight difference in silica content between tumour and surrounding tissue resulted in excellent contrast between tumour and tissue in MRI.

T2-W TSE image of the phantom



Imaging Parameters: TR = 2500 ms, TE = 52 ms, FA = 180°, ETL = 12, FOV = 260 x 260 x 10 mm<sup>3</sup>, matrix size = 128 x 128, and NEX = 2.

Estimated relaxation times


P dwhlde#	W4# p v/#	W5# p v/#
Wxp rufp p lf# -9#( #lj du## 7#( #vldf.#	53<<#	69#
Edfnj urxqg# p dwhlde# -9# 2y#lj du#	5469#	73#

## RESULTS

Based on coronal images showing the transducer and tumour/tissue it was possible to precisely move the FUS beam within the phantom. MR temperature was detected within the tumour and outside the tumour.

Coronal  
view

Indicative thermal maps acquired during and after sonication within the tumour mimic (coronal plane):

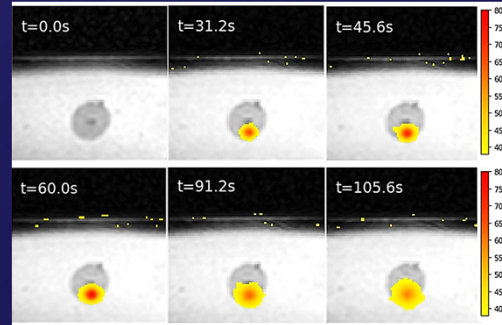


Coronal thermal maps extracted from FLASH images. Imaging parameters: TR=25 ms, TE=10 ms, FOV = 280x280x3 mm<sup>3</sup>, NEX = 1, FA = 30°, ETL = 1, matrix = 96 x 96. Sonication parameters: acoustic power = 60 W, duration = 60 s, and focal depth = 35 mm at 2.4 MHz.

ultraC@n

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

## RESULTS

Indicative thermal maps acquired during and after sonication within the tumour mimic (axial plane):

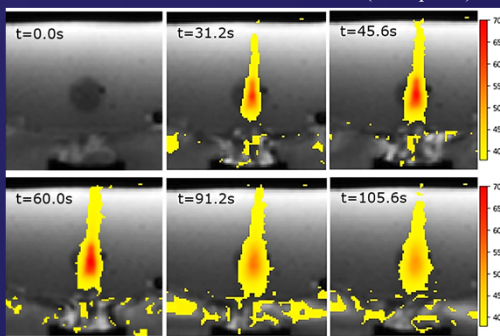

Axial thermal maps extracted from FLASH images. Imaging parameters: TR=25 ms, TE=10 ms, FOV = 280x280x3 mm<sup>3</sup>, NEX = 1, FA = 30°, ETL = 1, matrix = 96 x 96. Sonication parameters: acoustic power = 60 W, duration = 60 s, and focal depth = 35 mm at 2.4 MHz.


A peak temperature of 75 °C was estimated by MR thermometry within the tumour, whereas outside of the tumour a smaller peak temperature of 65 °C was recorded (baseline of 37 °C).

ultraC@n

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

## CONCLUSIONS

Due to the inclusion of silica in the tumour, the absorption was increased within the tumour, and therefore, higher temperatures were measured in the tumour. Temperature across a plane parallel to the beam showed some deflection of the beam in areas of tumour curvature. This is an excellent tumour model that can be used to evaluate the physics of focused ultrasound.

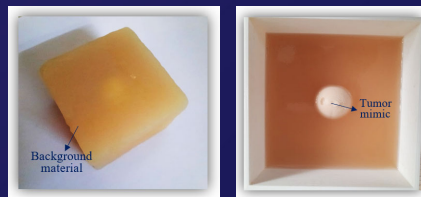

ultracon

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

## ACKNOWLEDGEMENTS

The study was funded by the Research and Innovation Foundation of Cyprus under the projects:  
SOUNDPET (INTEGRATED/0918/0008)  
FUSVET (SEED/1221/0080)



ultracon

AMERICAN INSTITUTE OF ULTRASOUND IN MEDICINE

Cyprus  
University of  
Technology

# MRI guided focused ultrasound system for veterinary oncology



Damianou C.,<sup>1</sup> Spanoudes K.,<sup>2</sup>

## INTRODUCTION

In this study, we investigated the ability of Focused Ultrasound (FUS) to precisely ablate targets mimicking canine and feline tumours using a Magnetic Resonance guided FUS (MRgFUS) robotic system. This modality could be an alternative therapeutic tool beyond traditional approaches.

## METHODS

Agar based targets were ablated with a MRgFUS robotic system featuring a single element spherically focused transducer of 2.7 MHz. The robotic system includes 3 linear cartesian axes.

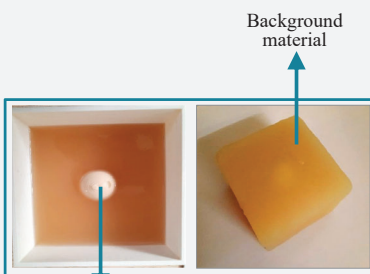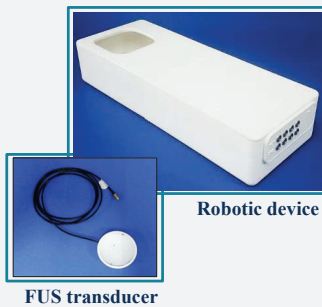

The tumour simulator was made of water, agar and silica, whereas in the material surrounding the tumour no silica was used.

The tumour mimicking phantom was imaged in a 3T MRI scanner (Magnetom Vida, Siemens Healthineers).


MR thermometry maps were produced to assess the thermal evolution during FUS sonications.



Experimental setup for phantom sonication in the 3T MRI scanner.

## RESULTS


The tumour simulator was visualized by MRI with excellent contrast from the surrounding material.



T2-W TSE image of phantom (TR = 2500 ms, TE = 52 ms, FA = 180°, ETL = 12, FOV = 260 x 260 x 10 mm<sup>3</sup>, matrix size = 128 x 128, and NEX = 2).

Based on coronal images of the transducer and tumour, it was possible to precisely move the FUS beam within the phantom. The MRgFUS system was capable of producing ablative temperatures within the tumour mimics.


### Indicative example of single sonication:

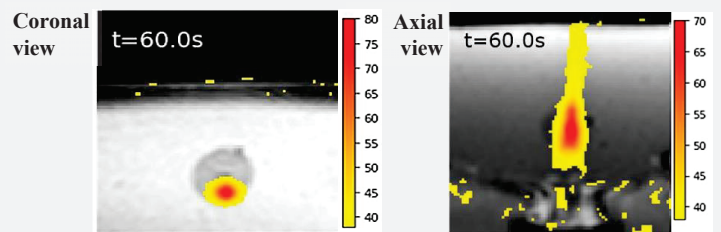

Thermal maps acquired at the end of sonication (60 W acoustic power, 60-s duration, 35-mm focal depth) in the tumour mimic extracted from FLASH images (TR=25 ms, TE=10 ms, FOV = 280x280x3 mm<sup>3</sup>, NEX = 1, FA = 30°, ETL = 1, matrix = 96 x 96).

A peak temperature of 75°C was recorded within the tumour (baseline of 37°C) using acoustic power of 60 W for 60 s.

### Indicative example of grid sonication:

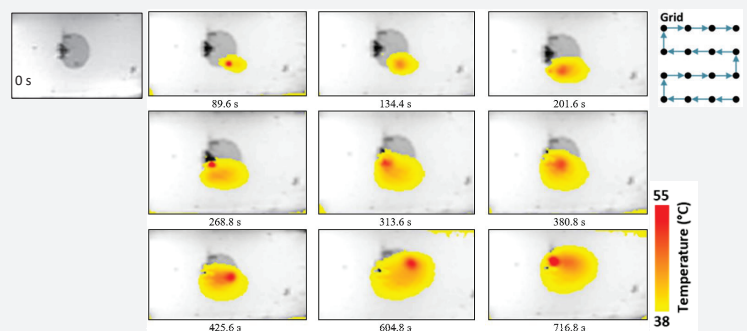

Indicative thermal maps acquired during sonication (45 W acoustic power, 30-s duration, 40-mm focal depth) in 4x4 grid (10-mm step, 30-s delay) in the tumour mimic extracted from FLASH images (TR=25 ms, TE=10 ms, FOV = 280x280x10 mm<sup>3</sup>, NEX = 1, FA = 30°, ETL = 1, matrix = 128x128).

## CONCLUSIONS

This technology has potential as a therapeutic solution for veterinary cancer. Although the device is MRI compatible, it can be used also outside the MRI setting using ultrasonic imaging. The next step is to apply this technology in animals and in humans.

The study was funded by the Research and Innovation Foundation of Cyprus under the projects:

FUSVET (SEED/1221/0080)  
SOUNDPET (INTEGRATED/0918/0008)



# T1 and T2 values of an Agar-based phantom with inclusion of tumour

Damianou C.,<sup>1</sup> Spanoudes K.,<sup>2</sup>




<sup>1</sup>PhD, Professor, Cyprus University of Technology, Limassol, Cyprus  
<sup>2</sup>DVM, PhD student, VET EX MACHINA LTD, Nicosia, Cyprus



## INTRODUCTION

An agar-based mimicking material which includes a tumour was developed. The phantom can be used to evaluate the temperature produced by a focused ultrasound (FUS) transducer.

## METHODS



phantom



FUS robotic device

The tumour model is composed of water, agar and silica. In the tissue surrounding the tumour no silica was included.

The T1 and T2 relaxation times of the phantom were measured in a 3T Magnetic Resonance Imaging (MRI) scanner (Magnetom Vida, Siemens Healthineers). Sonications were carried out with an MRI compatible FUS robotic system featuring a single element spherically focused transducer. The temperature was detected within the tumour and outside of the tumour by MR thermometry.

## CONCLUSIONS

Due to the inclusion of silica in the tumour the absorption was increased within the tumour, and therefore, higher temperatures were measured in the tumour. Temperature across a plane parallel to the beam showed some deflection of the beam in areas of tumour curvature. This is an excellent tumour model that can be used to evaluate the physics of the FUS technology.

## ACKNOWLEDGEMENTS

The study was funded by the Research and Innovation Foundation of Cyprus under the projects: FUSVET (SEED/1221/0080) SOUNDPET (INTEGRATED/0918/0008)



Ευρωπαϊκή Ένωση  
Ευρωπαϊκό Διαρθρωτικό και Επενδυτικό Ταμείο



Κυπριακή Δημοκρατία





Διαρθρωτικό Ταμείο της Επιστημονικής Ένωσης στην Κύπρο

## RESULTS

The slight difference in silica content between tumour and surrounding tissue resulted in excellent tumour visualization in MRI. The tumour mimic showed lower relaxation times owing to the addition of silica.

### Indicative results of T1 and T2 mapping:

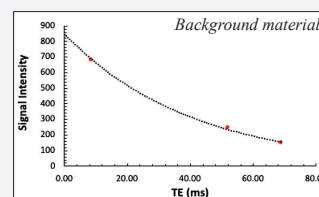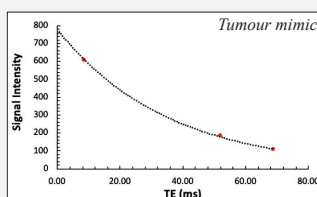

Signal intensities measured from T2-W Turbo Spin Echo (TSE) images using varied Echo time (TE) values for T2 mapping.


Material	T1 (ms)	T2 (ms)
Tumour mimic	2099.2	35.7
Background material	2135.8	40.0

**T2 mapping:** T2-W TSE sequence with varying TE values of 8 to 69 ms (TR = 250 ms, FA = 180°, FOV = 260 × 260 × 10 mm<sup>3</sup>, matrix size = 128 × 128, NEX = 2, ETL = 12).  
**T1 mapping:** Gradient Echo (GRE) sequence with varying FA values of 3 to 15° (TR = 15 ms, TE = 1.93 ms, FOV = 250 × 250 × 5 mm<sup>3</sup>, matrix size = 256 × 256, NEX = 1, ETL = 1).

Based on coronal images showing the transducer and tumour it was possible to precisely move the FUS beam within the phantom using the MR compatible positioning device.



transducer





tumour mimic

A maximum temperature of 65 °C was recorded outside of the tumour using acoustic power of 60 W for 60 s. A higher temperature of 75°C was reached within the tumour (baseline of 37°C).

**T2-W TSE images** (TR = 2500 ms, TE = 52 ms, FA = 180°, ETL = 12, FOV = 260 × 260 × 10 mm<sup>3</sup>, matrix size = 128 × 128, and NEX = 2).

Sonication within the tumour t=60 s Sonication outside of the tumour

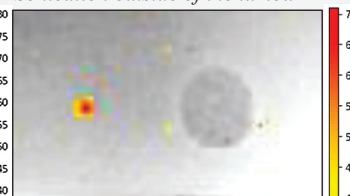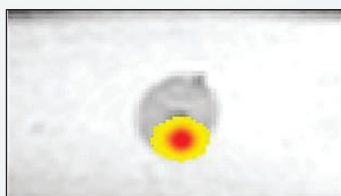

**Thermal coronal maps** acquired at the end of sonication (60 W acoustic power, 60-s duration, 35-mm focal depth) extracted from FLASH images (TR = 25 ms, TE = 10 ms, FOV = 280 × 280 × 3 mm<sup>3</sup>, NEX = 1, FA = 30°, ETL = 1, matrix = 96 × 96).



kyriakos.spanoudes@gmail.com  
christakis.damianou@cut.ac.cy

1-2 APRIL 2023  
**VETERINARY FORUM**  
**ON COMPANION ANIMAL MEDICINE**  
 PORTO PALACE HOTEL, THESSALONIKI



Canine and Feline  
**Geriatrics**

www.hcavs.gr

# Treatment of cancer with focused Ultrasound in cats and dogs

A. Antoniou, N. Evripidou, K. Spanoudes, C. Damianou\*  
Electrical Engineering Department, Cyprus University of Technology, Cyprus  
\* Corresponding author

## OBJECTIVES

The current study is a feasibility study using MRI guided focused ultrasound (FUS) for canine and feline cancer therapy using an existing preclinical MRI-compatible FUS robotic system.

## METHODS

FUS was delivered by a 2-MHz MRI compatible single-element spherically focused ultrasonic transducer which was integrated with an existing robotic positioning device with 4 computer-controlled axes. The functionality of the FUS system and sonication protocol in efficiently and safely ablating live tissue was initially validated in a rabbit thigh model in laboratory environment.

### Pet trials




For the pet trials, the treatment protocol included partial tumor ablation and was adjusted based on the tumor size. The motion and ultrasonic parameters were controlled through a dedicated FUS software. Post-sonication the tumors were removed and sent for histological examination.


## RESULTS

The system was capable of accurately delivering FUS to ablate live rabbit tissue. Both discrete and overlapping lesions of variable dimensions were inflicted in rabbit thigh by adjusting the ultrasonic parameters and spatial step between adjacent sonications.

### Typical results of rabbit thigh ablation

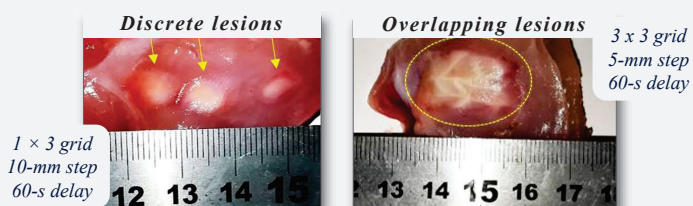

Top photos of rabbit thigh after muscle exposure. Sonications at 60 W (focal intensity of 2116 W/cm<sup>2</sup>) for 10 s at 1-cm focal depth.




Thermal lesion on mammary tumor using 45 W (focal intensity of 1590 W/cm<sup>2</sup>) for 20 s.

Nine (9) dogs and cats with superficial mammary cancer were recruited through a national champagne, according to set safety criteria. The veterinary patients underwent FUS ablation followed by immediate surgical resection of the tumor. All procedures were implemented successfully, with no recorded adverse events.

Hematoxylin and eosin (H&E) staining showed well-defined necrotic regions in all treated tumors. Red blood cell extravasation was observed at the lesion borderline in one case.

### Indicative histological slides

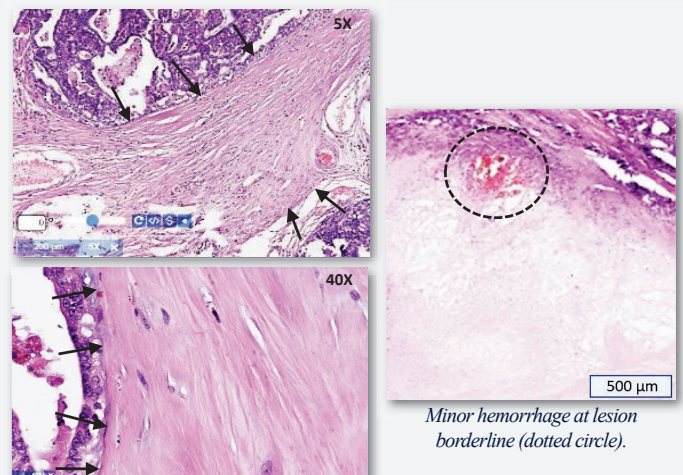

Black arrows delineate the area of necrosis. Sonications at 60 W (focal intensity of 2116 W/cm<sup>2</sup>) for 10 s at 2.5-cm focal depth.

## CONCLUSIONS

FUS ablation of mammary cancer under proper monitoring was proven safe and feasible. The FUS robotic system and related software offered an efficient procedural workflow. Further study with a larger patient population is needed to confirm the findings and demonstrate the feasibility of thermal FUS to safely ablate the entire tumor volume, as well as deep seated tumors.

## ACKNOWLEDGEMENTS

The study was funded by the Research and Innovation Foundation of Cyprus under the projects: SOUNDPET (INTEGRATED/0918/0008) FUSVET (SEED/1221/0080).





## ULTRASOUND AND MRI GUIDED FOCUSED ULTRASOUND SYSTEM FOR VETERINARY APPLICATIONS

Nikolas Evripidou, Anastasia Antoniou, *Christakis Damianou\**

Department of Electrical engineering, Computer engineering and Informatics


Cyprus University of Technology



*\*Corresponding author*

## ROBOTIC SYSTEM

**Magnetic Resonance-Guided Focused Ultrasound (MRgFUS) robotic system for preclinical applications.**

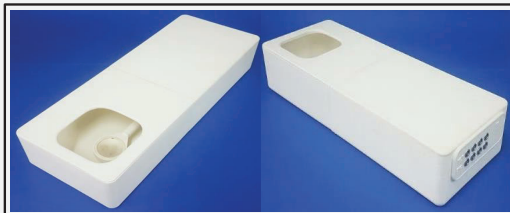

### Main features:

- ❑ 3D printed (F270, Stratasys, USA).
- ❑ 4 computer-controlled motion axes.
- ❑ Dimensions: 57 cm (L) x 21 cm (W) x 11.5 cm (H)
- ❑ MRI compatible materials.



## ROBOTIC SYSTEM

### Motion principle:

- Actuated by piezoelectric motors (USR30-S3N, Shinsei, Japan).
- Controlled by optical encoders (US Digital Corporation, USA).



### FUS transducer:

- Single element spherically-focused ultrasonic transducer
- 2-MHz central frequency.
- MRI compatible.

### MRgFUS software:

- Remote control of robotic motion and ultrasonic parameters.
- Treatment planning/ monitoring capabilities.




3

## SYSTEM EVALUATION IN A RABBIT THIGH MODEL

### Experimental protocol:

- FUS ablation of rabbit thigh under continuous anesthesia.
- Grid sonications with varying ultrasonic and grid parameters.

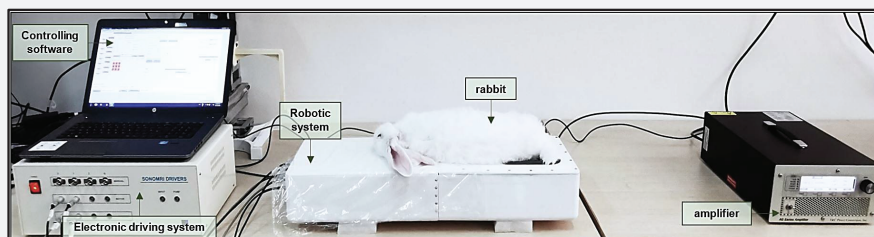

study license: CY/EXP/PR.L01/2020




4

## SYSTEM EVALUATION IN A RABBIT THIGH MODEL

- ❑ The system was capable of accurately delivering FUS to ablate live rabbit tissue.
- ❑ Discrete & overlapping lesions of variable dimensions were inflicted in tissue.
- ❑ Rabbit experiments provided proof of safety ⇒ Recruitment of pets (dogs/cats).

### Typical results of rabbit thigh ablation:

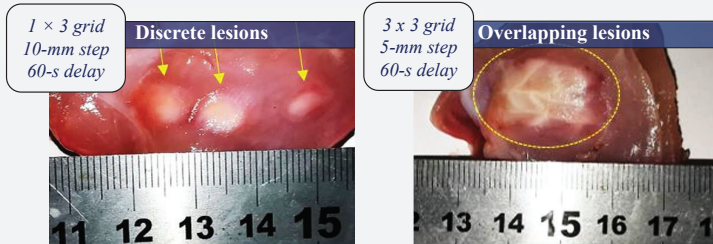

Top photos of rabbit thigh after muscle exposure. Sonications at 60 W; focal intensity of 2116 W/cm<sup>2</sup> for 10 s at 1-cm focal depth.

study license: CY/EXP/PR.L01/2020



5

## FEASIBILITY STUDY IN CANINE /FELINE CANCER PATIENTS

Nine (9) dogs and cats with superficial mammary cancer were recruited through a national champagne.

### Treatment protocol:

- ❑ Partial tumor ablation using high intensity FUS.
- ❑ Single OR Grid sonications depending on tumor size.
- ❑ Tumor excision following FUS.
- ❑ Histological examination.



Animal placement on the device at veterinary premises.

study license: CY/EXP/PR.L01/2020/R1/2021



6

## FEASIBILITY STUDY IN CANINE /FELINE CANCER PATIENTS

### Outcomes:

- All procedures were implemented successfully.
- NO recorded adverse events.
- Well-defined lesions were observed on tissue.



Lesion inflicted on mammary tumor using 45 W (focal intensity of  $1590\text{ W/cm}^2$ ) and sonication duration of 20 s.

study license: CY/EXP/PR.L01/2020/R1/2021




7

## FEASIBILITY STUDY IN CANINE /FELINE CANCER PATIENTS

### Histological examination:

- Hematoxylin and eosin (H&E) staining showed well-defined necrotic regions in all treated tumors.

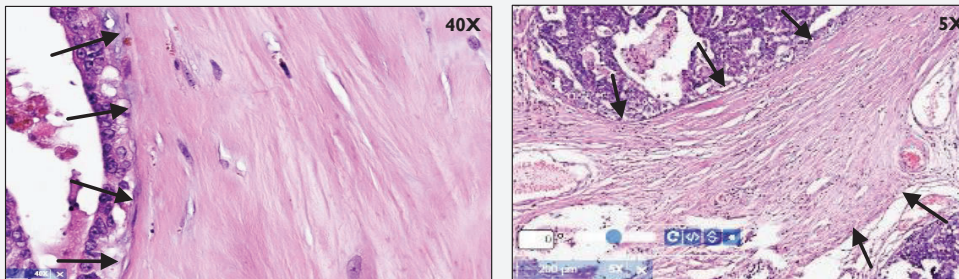

**Indicative histological slides:** Black arrows delineate the area of thermal necrosis. Sonications at 60 W (focal intensity of  $2116\text{ W/cm}^2$ ) for 10 s at 2.5-cm focal depth.

study license: CY/EXP/PR.L01/2020/R1/2021




8


## FEASIBILITY STUDY IN CANINE /FELINE CANCER PATIENTS

### Histological examination:

- ❑ Red blood cell extravasation was observed at the lesion borderline in one case.
- ❑ Intact cancer structures were observed occasionally within lesions.

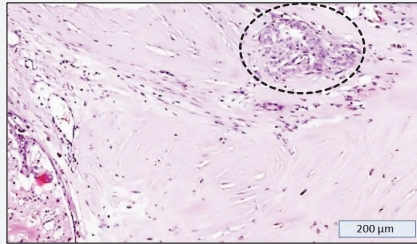

Intact cancer structure within the necrotic area (dotted circle).



Minor hemorrhage at lesion borderline (dotted circle).

study license: CY/EXP/PR.L01/2020/R1/2021



9

## CONCLUSIONS & FUTURE PROSPECTS


- ❑ **FUS ablation of mammary cancer** under proper monitoring was proven **safe and feasible**.
- ❑ The **FUS robotic system** offered an **efficient procedural workflow**.
- ❑ **Further study** is needed to:
  - ❑ Examine the phenomenon of **intact cancer structures**.
  - ❑ Assess the feasibility of **safely ablating the entire tumor volume & deep-seated tumors**.



10



**FUNDED BY:**



**PROJECTS:** SOUNDPET (INTEGRATED/0918/0008)  
FUSVET (SEED/1221/0080).

**PARTNERS:**



**ACKNOWLEDGEMENTS**



**Thank you for your attention!**



**christakis.damianou@cut.ac.cy**



# MR thermometry for a multipurpose phantom for focused ultrasound

Christakis Damianou\*, Nikolas Evripidou, Andreas Georgiou

Electrical Engineering Department, Cyprus University of Technology, Cyprus

\* christakis.damianou@cut.ac.cy




## OBJECTIVES


In this article we present our experience in acquiring thermal maps in a multipurpose phantom for a Focused Ultrasound (FUS) system operated under MRI monitoring.

## METHODS

An agar based phantom was used as the background tissue. The phantom contained a cyst mimic, a bone mimic, and a stone mimic.

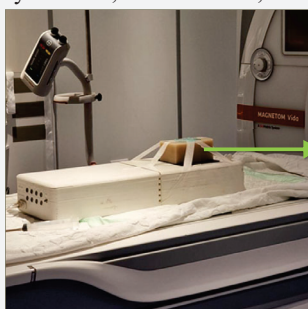

Agar-based phantom (6% w/v agar, 2% w/v silica)




A single element transducer was used operating at 2.7 MHz. The robotic system included 3 cartesian axes (X,Y,Z) and one angular axis. Phantom sonications were carried out in a Siemens Magnetom 3 T MRI scanner using acoustic power of 60 W for 60 s. MR thermometry was performed using a FLASH pulse sequence, which was optimized to provide noise-free temperature maps.

## RESULTS

- Sonication at 60 W for 60 s resulted in a focal temperature increase of 33.7°C, raising the phantom temperature to ablative levels.


Indicative thermal maps acquired during and after sonication in the phantom

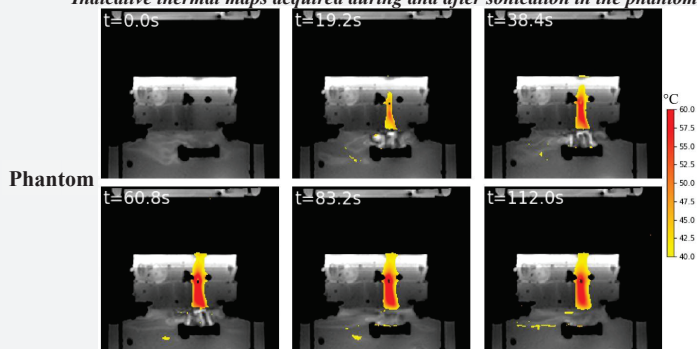

Axial thermal maps derived from FLASH sequence (TR = 25 ms, TE = 10 ms, slice thickness = 6 mm, flip angle = 30°, NEX = 1, Pixel bandwidth = 240 Hz/pixel, Matrix size = 128x128) during and after sonication at focal depth of 45 mm.

- The cyst mimic allowed ultrasound to pass, demonstrating a smooth increase in temperature, which was about 2-fold smaller ( $\Delta T = 16^\circ\text{C}$ ) than that observed in the phantom.


Indicative thermal maps acquired during and after sonication in the cyst mimic

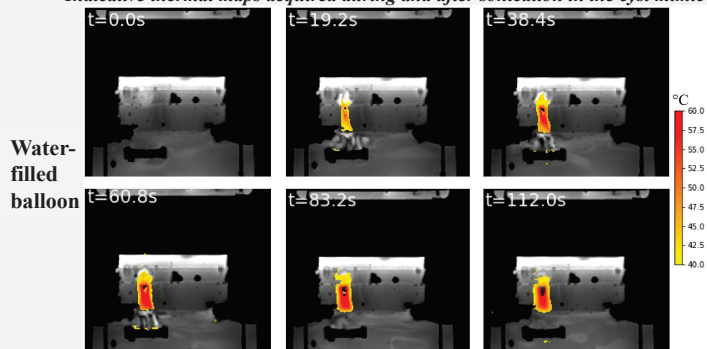


Axial thermal maps derived from FLASH sequence (TR = 25 ms, TE = 10 ms, slice thickness = 6 mm, flip angle = 30°, NEX = 1, Pixel bandwidth = 240 Hz/pixel, Matrix size = 128x128) during and after sonication at focal depth of 45 mm.

- It was found that the bone and stone mimic blocked ultrasound.

Indicative thermal maps acquired during and after sonication in the bone mimic

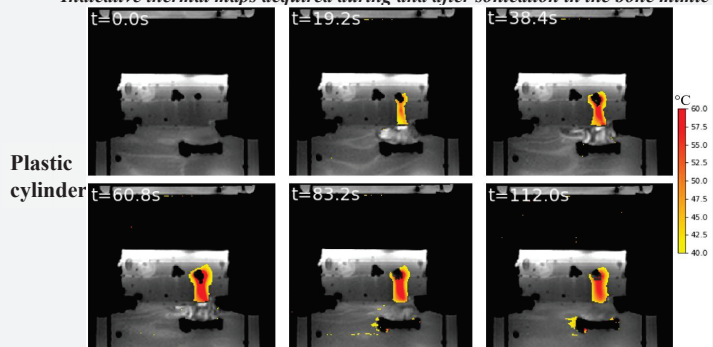

Indicative thermal maps acquired during and after sonication in the stone mimic

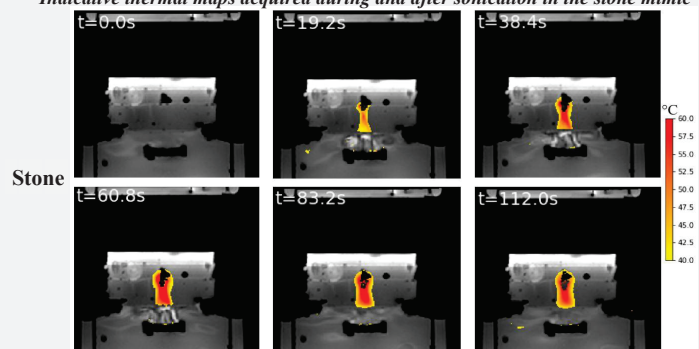

Axial thermal maps derived from FLASH sequence (TR = 25 ms, TE = 10 ms, slice thickness = 6 mm, flip angle = 30°, NEX = 1, Pixel bandwidth = 240 Hz/pixel, Matrix size = 128x128) during and after sonication at focal depth of 45 mm.

## CONCLUSIONS

This inexpensive phantom was proven successful in studying the penetration of focused ultrasound through these mimics. It could serve as a useful model for evaluating the physics of focused ultrasound.

## ACKNOWLEDGEMENTS

The study was co-funded by the European Structural & Investment Funds (ESIF) and the Republic of Cyprus through the Research and Innovation Foundation (RIF) under the projects SOUNDPET (INTEGRATED/0918/0008) and FUSVET (SEED/1221/0080).

