




DATE	DESCRIPTION OF CHANGE	APPV

1164 ISOLATION TRANSFORMER INSIDE OF THE GENERATOR
 S10, S11 PRESSURE SWITCHES LOCATED ON
 FRONT PANEL OF THE GENERATOR
 K295 PREHEAT CONTACTOR INSIDE OF GENERATOR
 K310 PLATE CONTACTOR INSIDE OF GENERATOR
 K4 CUT OUT RELAY

SHEET 1 OF 1	DATE 10/1/79	BY J. J. J.
UNIVERSAL 117V CONTROL WITH ANTI-TIE-DOWN MODULE INTERFACED WITH MANUAL SHUTTLE		
Gallman Co. MAG 1999		
DRAWING # 311000812		

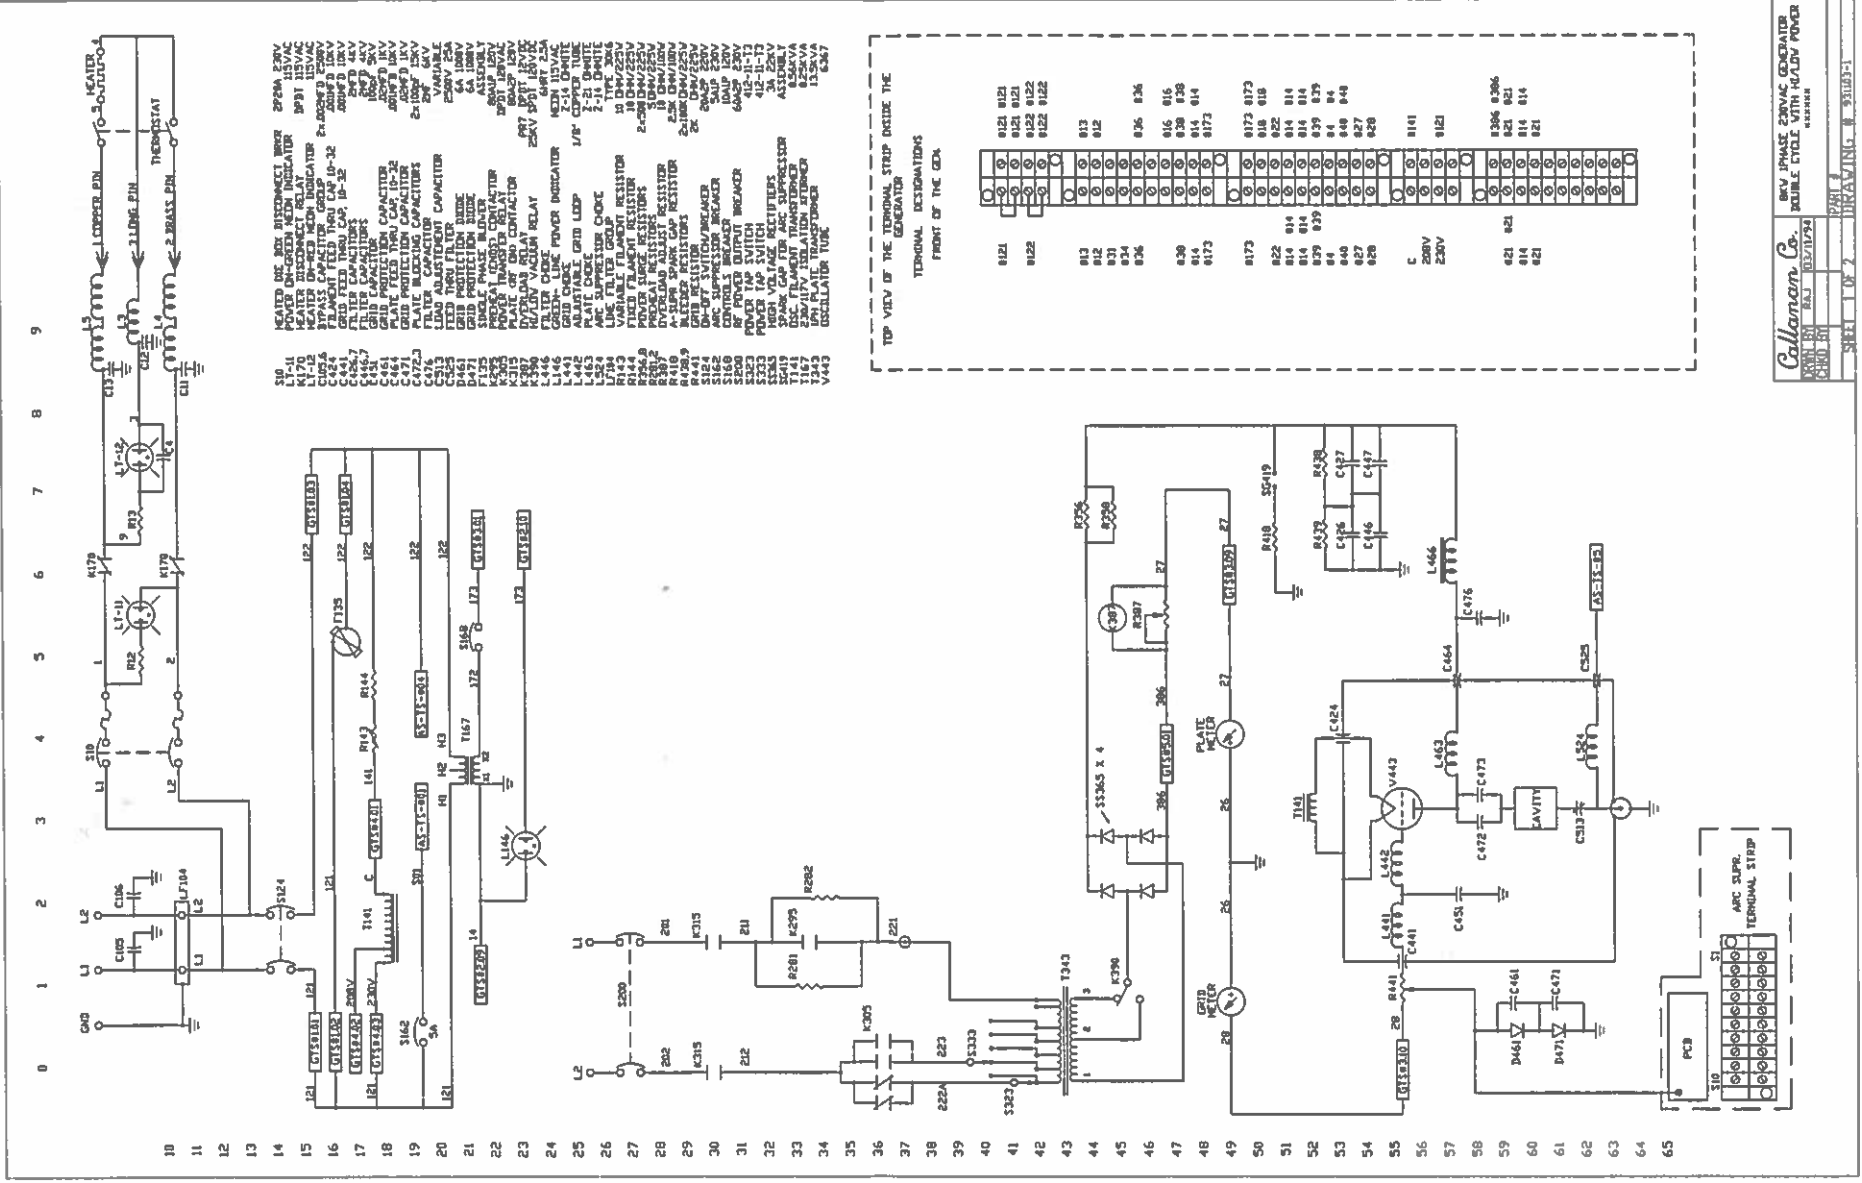